

**RANDOX**

**CARDIOLOGY & LIPID  
TESTING**

---



COMPLETE CARDIOLOGY & LIPID TESTING FROM RANDOX

**RANDOX**  
REAGENTS

## CARDIOLOGY & LIPID TESTING

Complete Cardiology and Lipid Testing from **Radox**

**RANDOX**

RANDOX LABORATORIES LTD.  
55 Diamond Road,  
Crumlin, County Antrim.  
BT29 4QY United Kingdom



1 x 19ml R1  
1 x 7ml R2



01	BENEFITS
02	INTRODUCTION
03	HDL CHOLESTEROL
05	LDL CHOLESTEROL
07	CHOLESTEROL
07	TRIGLYCERIDES
08	sdLDL CHOLESTEROL
09	LIPOPROTEIN (a)
11	APOLIPOPROTEIN A-I
11	APOLIPOPROTEIN A-II
11	APOLIPOPROTEIN B
12	APOLIPOPROTEIN C-II
12	APOLIPOPROTEIN C-III
12	APOLIPOPROTEIN E
13	sPLA <sub>2</sub> -IIA
14	HOMOCYSTEINE
15	MYOGLOBIN
15	DIGOXIN
16	DIAGNOSTIC BIOCHIP PRODUCTS
17	RESEARCH BIOCHIP PRODUCTS
18	ORDERING INFORMATION
20	REFERENCES
22	PORTFOLIO OF REAGENTS
23	GLOBAL DIAGNOSTIC SOLUTIONS PROVIDER
24	CONTACT US

#### KEY



#### NICHE PRODUCT

When you see this symbol you will know that Randox have one of the only **automated biochemistry assays** available on the market



#### UNIQUE FEATURE

When you see this symbol you will know that this feature is **unique to the Randox product**

## BENEFITS OF RANDOX REAGENTS

Randox offers an extensive range of third party diagnostic reagents which are internationally recognised as being of the highest quality; producing accurate and precise results.

We have a considerable test menu of over 100 assays, covering over 100 disease markers including: antioxidants, diabetes, drugs of abuse testing, lipids, specific proteins, therapeutic drug monitoring and veterinary testing.

A wide range of formats and methods are available providing greater flexibility and choice for any laboratory size.

In addition to flexible pack sizes and a comprehensive list of analyser applications, we can also provide dedicated reagent packs (Randox Easy Read and Easy Fit reagents) for a wide range of chemistry analysers providing you with freedom of choice from an independent manufacturer.



### EXPAND YOUR TEST MENU WITHOUT EXPANDING YOUR LAB

There is no need to buy any extra equipment in order to expand your test menu. Our reagents can be programmed onto the majority of the most common biochemistry analysers.



### EXPAND ROUTINE TESTING

With speciality assays for 195 of the most common clinical chemistry analysers; assays which usually require dedicated equipment (or was previously only available as an ELISA) can now be run on automated biochemistry analysers, allowing your laboratory to expand its routine test menu. E.g. TxBCardio™, H-FABP, adiponectin, and many more.



### REDUCE COSTS

The excellent quality and stability associated with Randox reagents helps to reduce costs by keeping waste and costly re-runs to a minimum.



### BRING TESTING IN-HOUSE

The availability of flexible pack sizes ensures suitability for laboratories of all sizes and means tests can easily be brought in-house without the worry of increased waste.



### REDUCE LABOUR

Reduce time spent running tests through liquid ready-to-use reagents, automated methods (compared to the traditional laborious ELISA methods used for tests such as cystatin C or adiponectin); and our easy-fit options.



### REDUCE THE RISK OF ERRORS AND HAVE CONFIDENCE IN PATIENT RESULTS


Our traceability of material and extremely tight manufacturing tolerances ensure uniformity across reagent batches reducing lot-to-lot variability. All our assays are validated against gold-standard methods; increasing confidence in patient test results.

**INTRODUCTION TO RANDOX CARDIOLOGY AND LIPID TESTING**


International bodies, including the National Lipid Association and the European Guidelines on Cardiovascular Disease (CVD) Prevention in Clinical Practice advocate measuring lipids to truly identify CVD risk. However, the traditional lipid panel of cholesterol, HDL-C, triglycerides and LDL-C only detect approximately 20% of all coronary artery disease (CAD) patients. Advanced lipid testing is recommended to optimise patient treatment, both in primary and secondary risk categories and as such provide the necessary tools to prevent and reduce the risks. Randox offers a comprehensive cardiology product profile which includes superior performing reagents for the detection of conventional risk factors, as well as emerging biomarkers associated with further risk.

**LIPOPROTEIN SUBFRACTIONS**

Fig. 1 The changes in density and diameter of the lipoprotein subfractions.<sup>1</sup>

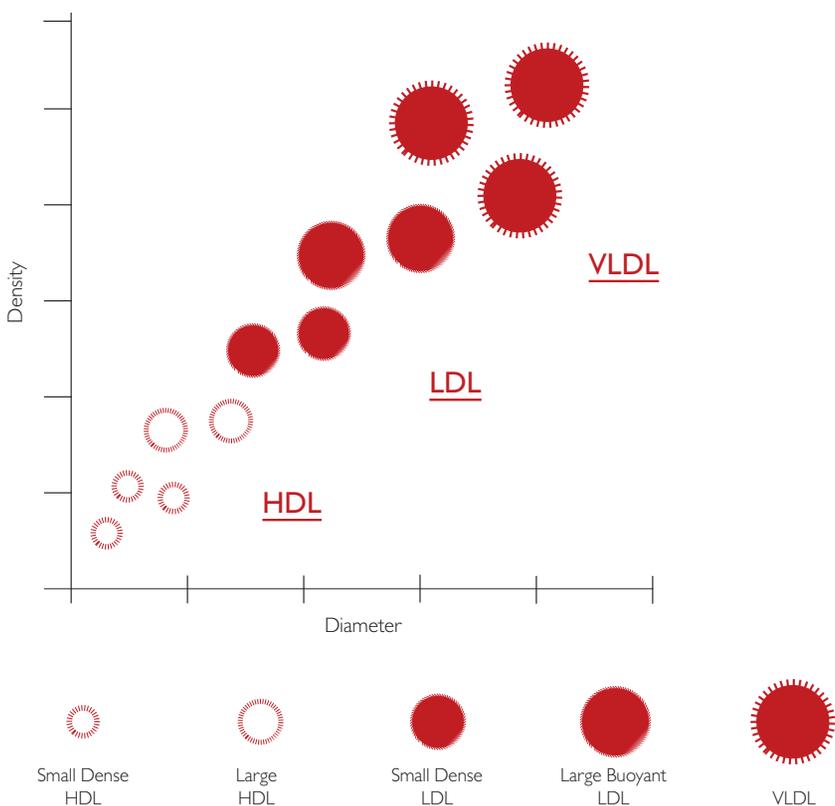

Please note this is a visual representation and is not drawn to scale.

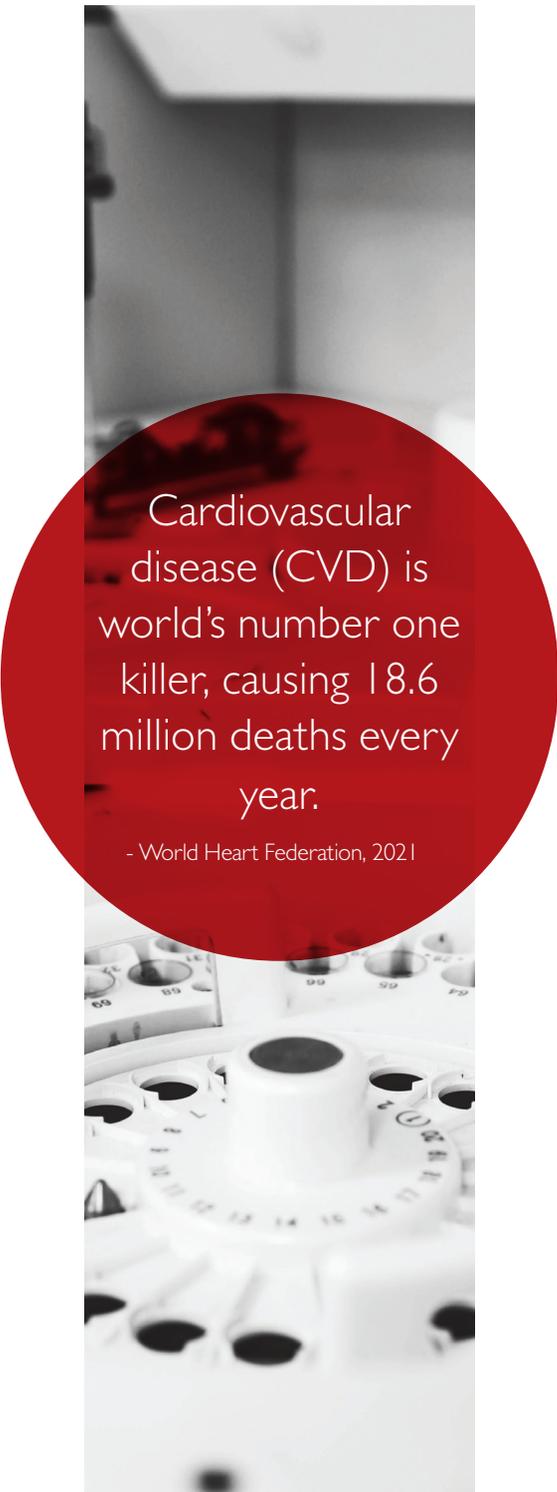

Cardiovascular disease (CVD) is world's number one killer, causing 18.6 million deaths every year.

- World Heart Federation, 2021



## HDL CHOLESTEROL

### Key Features of the Randox HDL Cholesterol Assay

- UF Superior direct clearance methodology** ensuring truly accurate results even with abnormal samples
  - **Liquid ready-to-use reagents** for convenience and ease of use
  - **Extensive measuring range** of 0.189 - 3.73mmol/L
  - **Applications available** detailing instrument-specific settings for the convenient use of the Randox HDL Cholesterol (HDL-C) assay on a wide range of clinical chemistry analysers

### UF Benefits of the Randox Direct Clearance Method

Although many direct methods of HDL-C measurement perform well with normal samples, they show reduced specificity and often underestimate the concentration of HDL-C in samples containing abnormal lipoproteins, for example, samples from patients with elevated triglyceride levels or liver damage. The Randox direct clearance method offers superior performance to these methods and works by completely removing all non-HDL-C components resulting in a high degree of accuracy and specificity with HL samples.


### Clinical Significance


High-density lipoproteins (HDL) are one of the major classes of plasma lipoproteins. HDL-C is often referred to as 'good cholesterol' as it transports from the tissues to the liver for removal from the body. High levels of HDL-C can lower the risk of developing heart disease.

### Performance in discrepant patient samples

Fig. 2 below compares the performance of the Randox direct clearance method and two other direct masking methods with the ultracentrifugation reference method in two abnormal samples. The Randox direct clearance method correlates well with the ultracentrifugation method; however the two other commercially available direct masking methods seriously underestimate the concentration of HDL-C.

Fig. 2 Randox Direct Clearance Method vs Direct Masking Methods.<sup>2</sup>

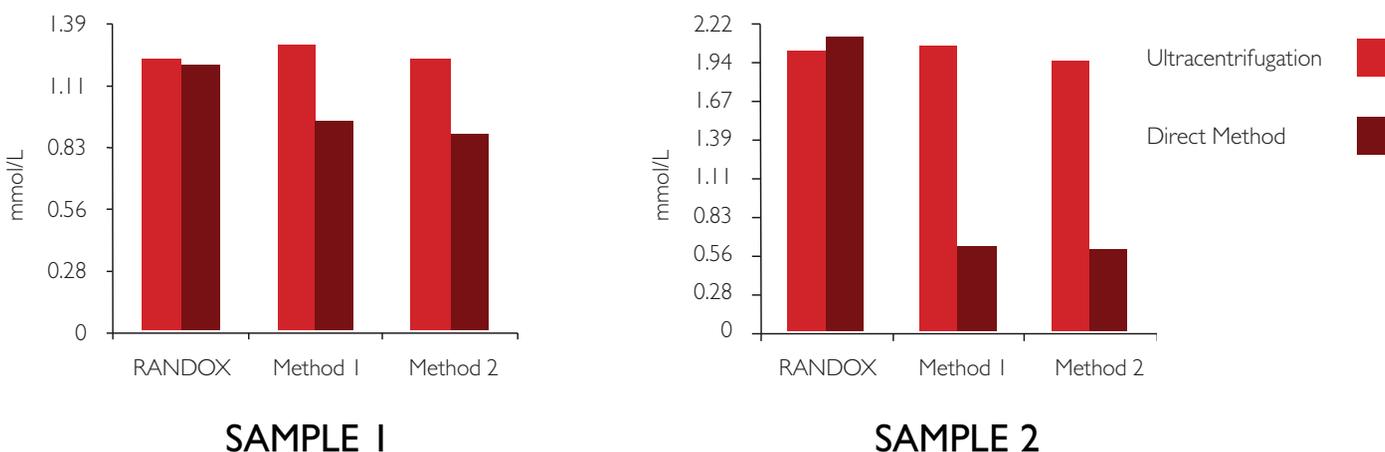

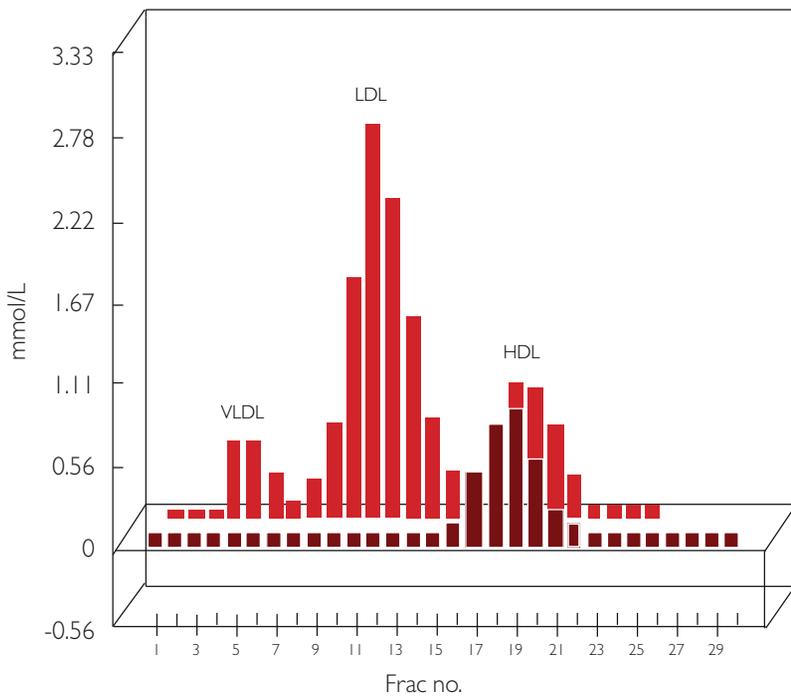

**Fig. 3 Specificity of Radox Direct Clearance Assay for HDL Cholesterol**

Specificity of the Radox direct clearance HDL-C assay was verified against gel filtration. Fig. 3 indicates how specific the Radox direct clearance method is for HDL-C. Our kit was found to only react with the HDL-C fractions separated by gel filtration.

Total Cholesterol Reagent



Radox HDL Cholesterol Reagent



“  
THE DIAGRAM ABOVE  
SHOWS HOW SPECIFIC  
THE RADOX DIRECT  
CLEARANCE METHOD IS  
”





## LDL CHOLESTEROL

### Key Features of the Randox LDL Cholesterol Assay

- **Superior direct clearance methodology** ensuring truly accurate results are delivered
  - **Liquid ready-to-use reagents** for convenience and ease-of-use
  - **Extensive measuring range** of 0.189 – 22.2mmol/L for the measurement of clinically significant levels
- UF** **Applications available** detailing instrument-specific settings for the convenient use of the Randox LDL Cholesterol (LDL-C) assay on a wide range of clinical chemistry analysers

### UF Benefits of the Randox Direct Clearance Method

The Randox direct clearance method eliminates sample pre-treatment, displaying an excellent correlation to both the ultracentrifugation and precipitation methods. The detergents and buffering systems used by most commercially available direct clearance LDL-C assays produce varying results, leading to differences in assay performance.

**Excellent precision** as the Randox LDL-C assay retains its precision even at high levels of triglycerides.

**Minimal interferences** as the Randox advanced reagent formulation enables rapid clearance of turbidity resulting in minimal interference from patient samples.

### Clinical Significance

LDL-C, often referred to as 'bad cholesterol', transports cholesterol to the tissues and is linked to the development of atherosclerotic lesions. The accurate measurement of LDL-C is therefore of vital importance in therapies which focus on lipid reduction to prevent or reduce the progress of atherosclerosis and to avoid plaque rupturing.

The traditional method of measuring LDL-C levels is through the empirical relationship of Friedewald. This equation uses quantitative measurements of total cholesterol, HDL-C and triglycerides to find a value for LDL-C. However, this equation has a number of limitations that have led to inaccuracies. The Randox LDL-C assay eliminates the limitations associated with Friedewald by utilising the direct clearance method, providing a more accurate diagnosis of patient samples.

Fig. 4 Mis-estimation of LDL-C by Calculation Method with Increasing Triglycerides



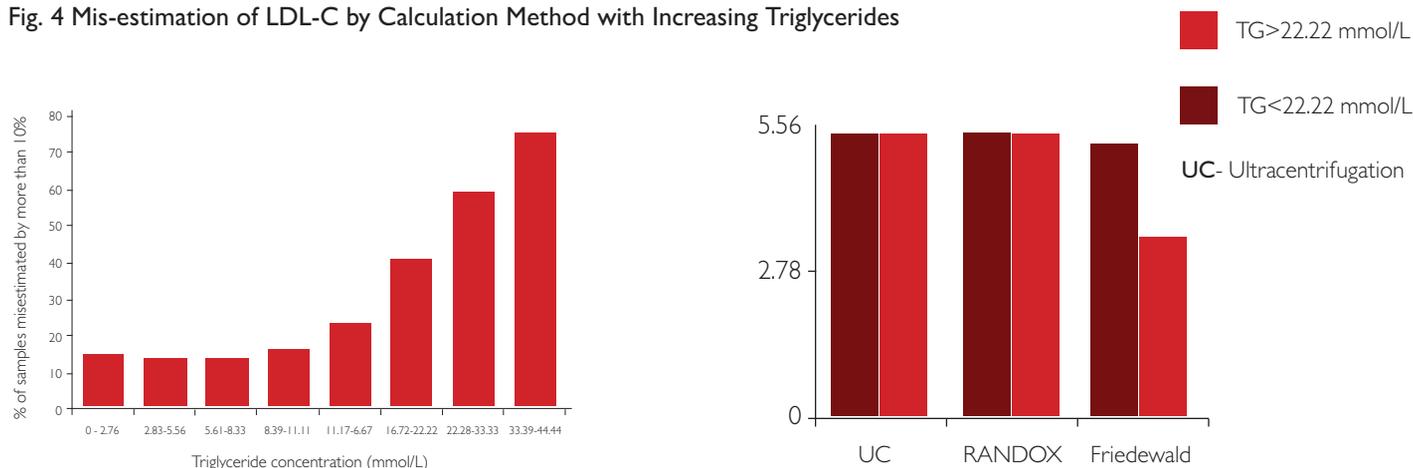


Fig. 4 shows the mis-estimation of LDL-C by the Friedewald equation with increasing triglycerides and how the Randox direct clearance method offers superior performance.

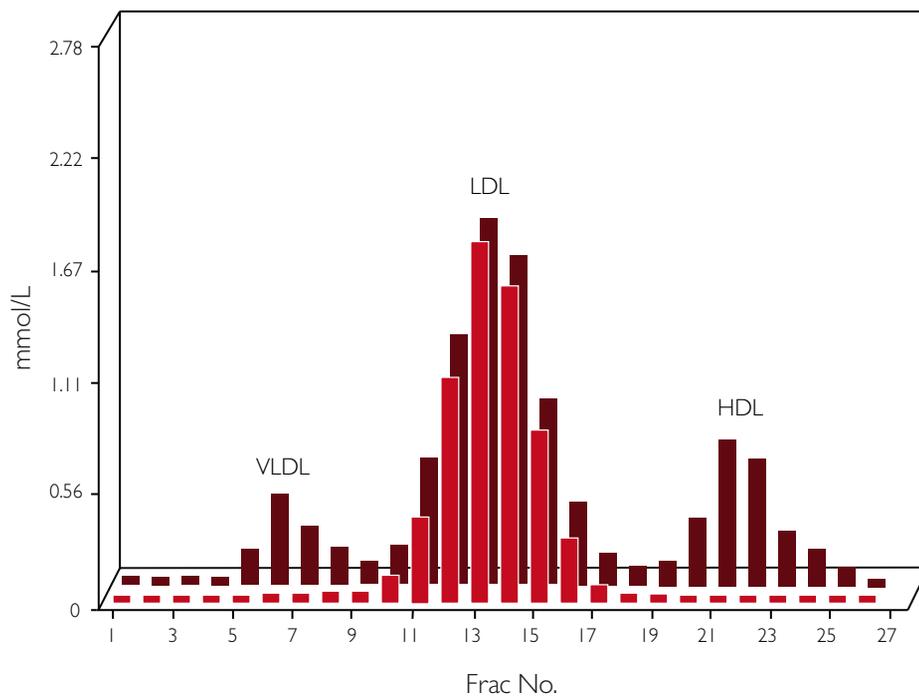

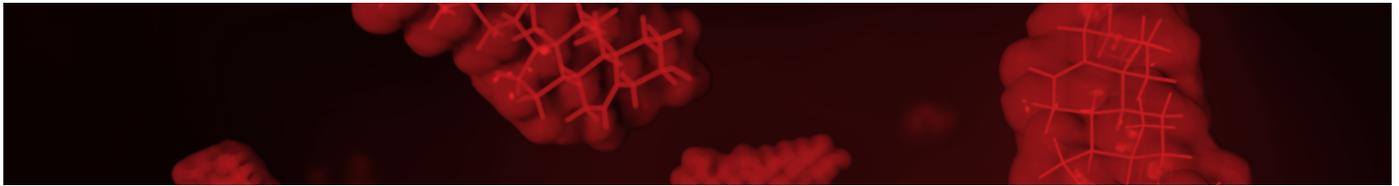


**Fig. 5 Specificity of the Radox Direct Clearance Assay for LDL Cholesterol**

Specificity of the Radox direct clearance LDL-C assay was verified against gel filtration. Fig. 5 indicates how specific the Radox direct clearance method is for LDL-C. Our kit was found to only react with the LDL-C fractions separated by gel filtration.

- Radox LDL Cholesterol
- Total Cholesterol



“  
 THE FRIEDEWALD  
 FORMULA HAS  
 BEEN REPORTED TO  
MISCLASSIFY UP TO  
50% OF PATIENTS<sup>3</sup>  
 ”

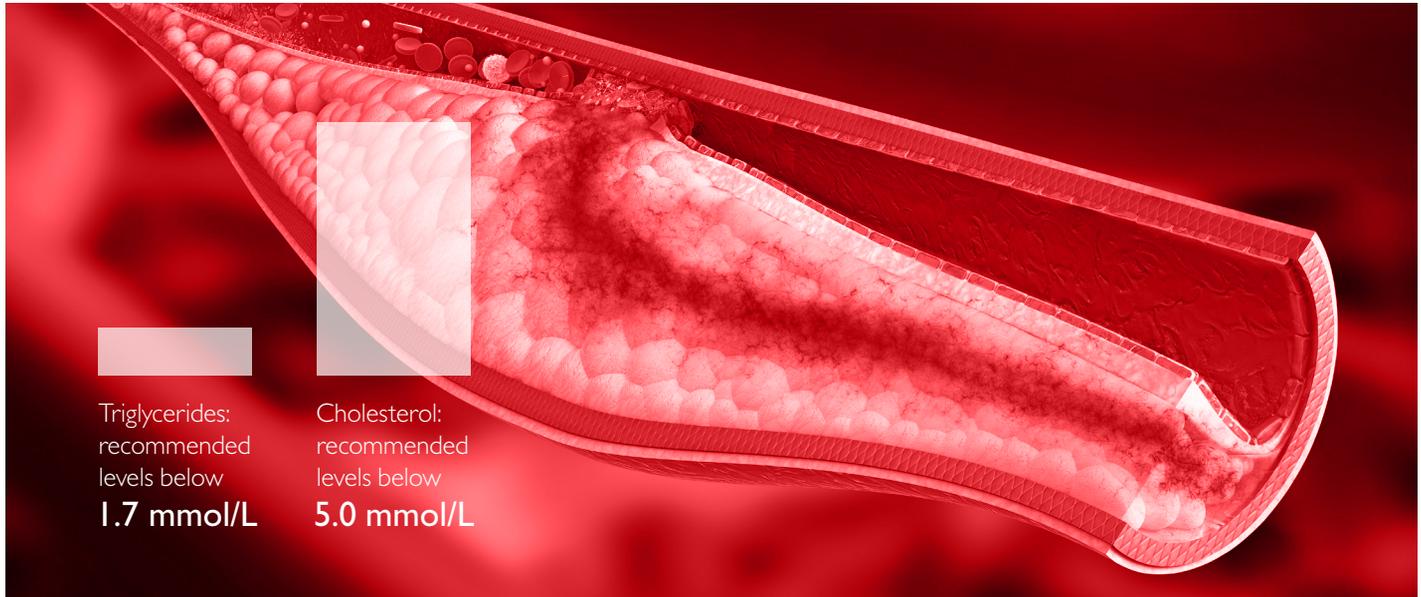

Triglycerides:  
recommended  
levels below  
**1.7 mmol/L**

Cholesterol:  
recommended  
levels below  
**5.0 mmol/L**

## CHOLESTEROL (TOTAL)

### Key Features of the Randox Cholesterol Assay

- **Wide range of kits available** ensuring laboratories of all sizes can find a product to suit their needs
- **Liquid ready-to-use reagents** for convenience and ease-of-use
- **Standards included in certain kits** for user convenience (these are for manual and semi-automated use only)
- **Extensive measuring range** of 0.865-16.6 mmol/L for the measurement of clinically significant levels
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Cholesterol assay on a wide range of clinical chemistry analysers
- **CHOD-PAP method**

### Clinical Significance

Total Cholesterol measures all lipoprotein sub-classes to assess a patient's overall cholesterol levels. Elevated levels of cholesterol in the blood are associated with atherosclerosis and an increased risk of heart disease. As such Total Cholesterol testing plays a vital role in preventative health care. Both the American National Cholesterol Education Programme (NCEP) and the European Society of Cardiologists (ESC) recommend levels below 5 mmol/L.

## TRIGLYCERIDES

### Key Features of the Randox Triglycerides Assay

- **Wide range of kit sizes and formats available** offering choice and minimal reagent waste
- **Liquid and lyophilised formats available** for greater choice
- **Standards included in certain kits** for user convenience (these are for manual and semi-automated use only)
- **Extensive measuring range** of 0.134-12.7 mmol/L for the measurement of clinically significant levels
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Triglycerides assay on a wide range of clinical chemistry analysers
- **GPO-PAP method**

### Clinical Significance

Elevated triglyceride levels increase the atherogenicity of HDL-C and LDL-C. A triglyceride concentration of less than 1.7 mmol/L is desirable. Levels higher than this are not only associated with an increased risk of heart disease but also type 2 diabetes, kidney disease, hypothyroidism and pancreatitis.




**NP SMALL-DENSE LDL CHOLESTEROL (sdLDL-C)**

**Key Features of the Randox sdLDL Cholesterol Assay**

Until recently, the primary methods of assessing a patient's sdLDL-C levels were based on techniques such as ultracentrifugation and electrophoresis both of which are extremely laborious and time-consuming. <sup>4</sup>sdLDL-C can now be assessed in the routine biochemistry laboratory using the Randox Clearance assay.

- **Randox sdLDL-C utilises the clearance method** which produces results in ten minutes. There are two main reaction steps based on the presence of surfactants and enzymes that selectively react with a certain group of lipoproteins
- **The Randox automated sdLDL-C assay correlates extremely well with the gold standard method** ultracentrifugation as shown in Fig. 6
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox sdLDL-C assay on a wide range of clinical chemistry analysers
- **Liquid ready-to-use reagents** for convenience and ease-of-use

**Fig. 6 Correlation of Ultracentrifugation and Denka Seiken Methods. <sup>6</sup>**

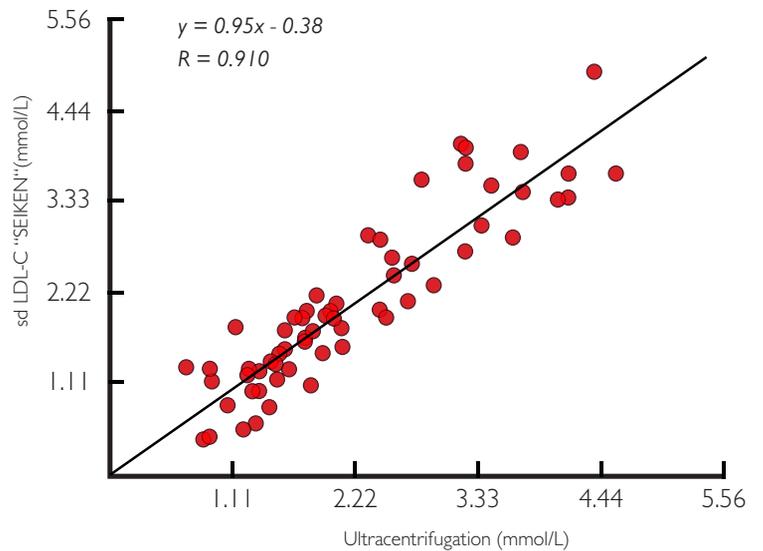

64 SAMPLES FROM HEALTHY PEOPLE, CAD & DIABETIC PATIENTS


**Clinical Significance**

When measuring LDL-C, you are measuring the cholesterol mass within LDL-C particles. The LDL particle population within LDL is heterogeneous - meaning that size, density & composition of each particle will be different. sdLDL-C is a subfraction of low density lipoprotein (LDL) with smaller particle size and higher density than larger more buoyant LDL-C. They all transport triglycerides and cholesterol to the tissues but their atherogenesis varies according to their size. sdLDL-C will more readily permeate the inner arterial wall has a lower affinity to the hepatic LDL-C receptor and as such circulates in the blood longer and is more susceptible to oxidation.

As sdLDL-C is particularly atherogenic, a person with elevated sdLDL-C levels has a 3-fold increased risk of myocardial infarction (MI).<sup>5</sup>

sdLDL-C measurement provides a more comprehensive understanding of the risk of lipoproteins within a patient. sdLDL-C measurement is more comprehensive in detecting cardiovascular risk compared to the traditional LDL-C test. Fig. 7 illustrates the predominance of sdLDL-C particles in comparison to LDL-C particles.<sup>7</sup>

**Fig. 7 Predominance of sdLDL-C particles in comparison to LDL-C particles.<sup>7</sup>**

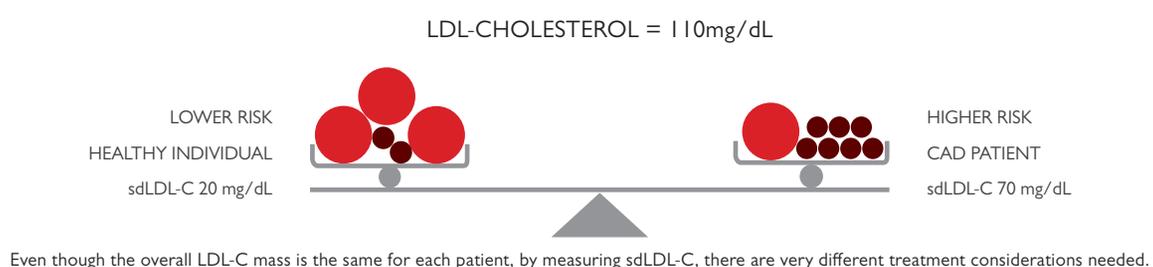



## LIPOPROTEIN (a) (Lp(a))

### Traditional challenges of Lp(a) measurement

The widespread use of Lp(a) as an independent risk factor for cardiovascular disease risk has, until recently, been impeded by the lack of internationally accepted standardisation and the fact that many commercial Lp(a) methods suffer from apolipoprotein (a) (apo(a)) size related bias, potentially leading to patient misclassification.

The size heterogeneity of apo(a) affects, to varying degrees the results of many commercially available Lp(a) kits. This may result in an underestimation of Lp(a) in samples containing apo(a) molecules smaller than that used in the assay's calibrator and conversely may overestimate the concentration in samples containing larger apo(a) particles.



### Criteria to overcome challenges of Lp(a) measurement

#### IFCC -

The International Federation of Clinical Chemistry (IFCC) Working Group on Lp(a) recommends that laboratories use assays which do not suffer from apo(a) size-related bias, in order to minimise the potential of risk misclassification of patients for coronary heart disease.

#### Lipoprotein(a) Foundation -

The Lp(a) Foundation has referenced Marcovina and Albers (2016)<sup>8</sup> as their recommendation for the best Lp(a) test. This study comes to the following conclusions:

- Robust assays based on the Denka method are available, which are reported in nanomoles per litre (nmol/L) and are traceable to WHO/IFCC reference material
- Five point calibrators with accuracy assigned target values will minimise the sensitivity to apo (a) size
- Upon request, manufacturers should provide the certificate of evaluation of the calibrator and reagent lots with the relative expiration dates

### Key Features of the Randox Lp(a) Assay

- UF** The Randox Lp(a) assay is one of the only methodologies on the market that detects the non-variable part of the Lp(a) molecule and therefore suffers minimal size related bias providing more accurate and consistent results. The Randox Lp(a) kit is standardised to the WHO/ IFCC reference material SRM 2B and is closest in terms of agreement to the ELISA reference method.
- UF** Five point calibrator with accuracy-based assigned target values are provided which accurately reflect the heterogeneity of isoforms present in the general population
- **Measuring units available in nmol/L upon request**
- **Highly sensitive and specific** method for Lp(a) detection in serum and plasma
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Lp(a) assay on a wide range of clinical chemistry analysers
- **Liquid ready-to-use reagents** for convenience and ease-of-use





## APOLIPOPROTEIN A-I


### Key Features of the Randox Apolipoprotein A-I Assay

- **Liquid ready-to-use reagents** for convenience and ease-of-use
- **Wide measuring range** of 6.50-233 mg/dL for the measurement of clinically important results
- **Limited interference** from Bilirubin, Haemoglobin, Intralipid® and Triglycerides, producing more accurate results
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Apolipoprotein A-I assay on a wide range of clinical chemistry analysers

### Clinical Significance

Apolipoprotein A-I is one of the main protein forms found in High Density Lipoproteins (HDL). The chief role of Apolipoprotein A-I is in the activation of lecithin cholesterol acyl transferase (LCAT) and the capture and removal of free cholesterol from extrahepatic tissues. This process is called reverse cholesterol transport. Apolipoprotein A-I may therefore be described as non-atherogenic, showing an inverse relationship to cardiovascular risk.

Studies have shown that there is an inverse relationship between Apolipoprotein A-I and coronary artery disease (CAD), whereas Apolipoprotein B has a direct relationship with CAD. Patients with CAD generally display reduced levels of Apolipoprotein A-I and increased levels of Apolipoprotein B.

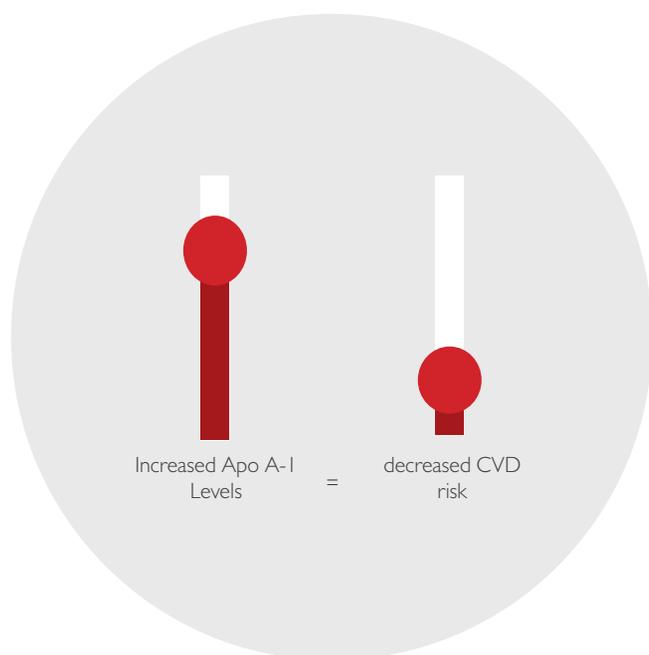

## APOLIPOPROTEIN A-II

### Key Features of the Randox Apolipoprotein A-II Assay

- **Liquid ready-to-use reagents** for convenience and ease-of-use
- **Wide measuring range** of 6.75-61.1 mg/dL for the measurement of clinically important results
- **Limited interference** from Bilirubin, Haemoglobin, Intralipid® and Triglycerides, producing more accurate results
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Apolipoprotein A-II assay on a wide range of clinical chemistry analysers

### Clinical Significance

Apolipoprotein A-II is a major constituent of HDL-C particles and plays an important role in the processes of reverse cholesterol transport and lipid metabolism. The increased production of Apolipoprotein A-II promotes atherosclerosis by decreasing the proportion of anti-atherogenic HDL-C containing Apolipoprotein A-I.

## APOLIPOPROTEIN B


### Key Features of the Randox Apolipoprotein B Assay

- **Liquid ready-to-use reagents** for convenience and ease of use
- **Extensive measuring range** of 11.2-184 mg/dL for the measurement of clinically important results
- **Limited interference** from Bilirubin, Haemoglobin, Intralipid® and Triglycerides, producing more accurate results
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Apolipoprotein B assay on a wide range of clinical chemistry analysers

### Clinical Significance

Apolipoprotein B is the main form of protein found in Low Density Lipoproteins (LDL). Apolipoprotein B shows atherogenic signs and is therefore useful in the evaluation of coronary risk. Elevated levels of Apolipoprotein B indicate increased cardiovascular risk even when total and LDL cholesterol levels are shown to be within the normal range, making this an important risk marker.

Apolipoprotein B is often tested alongside Apolipoprotein A-I to determine the Apolipoprotein B / Apolipoprotein A ratio which can be used as an alternative to the Total Cholesterol /HDL Cholesterol ratio when determining cardiovascular risk.

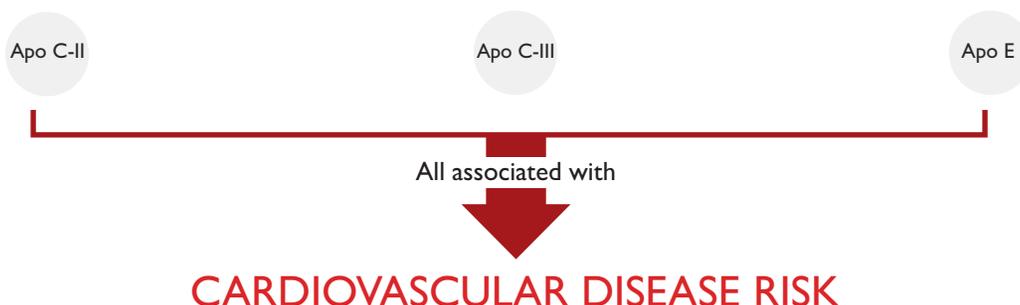

**(NP) APOLIPOPROTEIN C-II**

**Key Features of the Randox Apolipoprotein C-II Assay**

- **Liquid ready-to-use reagents** for convenience and ease-of-use
- **Excellent sensitivity** of 1.48 mg/dL, ensuring depleted levels of Apo C-II are detected
- **Limited interference** from Bilirubin, Haemoglobin, Intralipid® and Triglycerides, producing more accurate results
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Apolipoprotein C-II assay on a wide range of clinical chemistry analysers

**Clinical Significance**

Apolipoprotein C-II deficiency can lead to hypertriglyceridemia in patients; therefore measuring Apolipoprotein C-II can be used as an aid in assessing CVD risk. Apolipoprotein C-II deficient patients present with chylomicronemia, xanthomas, and recurrent pancreatitis.

**(NP) APOLIPOPROTEIN C-III**

**Key Features of the Randox Apolipoprotein C-III Assay**

- **Liquid ready-to-use reagents** offering optimum convenience and ease-of-use
- **Excellent linearity** of 21.7 mg/dL. The approximate normal upper limit for Apo C-III is 9.5 mg/dL, therefore the Randox assay will comfortably detect elevated, potentially harmful levels of Apo C-III
- **Limited interference** from Bilirubin, Haemoglobin, Intralipid® and Triglycerides, producing more accurate results
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Apolipoprotein C-III assay on a wide range of clinical chemistry analysers

**Clinical Significance**

Apolipoprotein C-III modulates the uptake of triglyceride-rich lipoproteins by the LDL receptor related protein through inhibition of lipoprotein lipase. Elevated levels of Apolipoprotein C-III are associated with both primary and secondary hypertriglyceridemia.

Genetically determined Apolipoprotein C-III deficiency has shown to increase the rate of triglyceride clearance from the plasma **up to 7-fold**. Apolipoprotein C-III levels have been reported higher in many conditions including type 2 diabetes, hyperbilirubinemia, kidney deficiency and decreased thyroid function. Factors that can influence Apolipoprotein C-III levels include gender, age, menopause and genetic polymorphisms in the Apolipoprotein C-III gene.

**(NP) APOLIPOPROTEIN E**

**Key Features of the Randox Apolipoprotein E Assay**

- **Liquid ready-to-use reagents** for convenience and ease-of-use
- **Extensive measuring range** of 1.04-12.3 mg/dL for measurement of clinically important results
- **Limited interference** from Bilirubin, Haemoglobin, Intralipid® and Triglycerides, producing more accurate results
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Apolipoprotein E (Apo E) assay on a wide range of clinical chemistry analysers

**Clinical Significance**

Apo E is an amino acid which has many functions including the transport of triglycerides to the liver tissue and distribution of cholesterol between cells.

A deficiency in Apo E gives rise to high serum cholesterol and triglyceride levels and as a result, leads to premature atherosclerosis. A number of factors can affect Apo E concentrations including: the genetic polymorphism, oral contraceptive intake, puberty, BMI and age.



NP sPLA<sub>2</sub>-IIA



Biological Significance of sPLA<sub>2</sub>-IIA

The secretory phospholipase A<sub>2</sub> family comprises of a large range of enzymes whose main function is to hydrolyse phospholipids from the cell membrane surface and lipoproteins.<sup>15</sup> sPLA<sub>2</sub>-IIA is thought to be the most highly expressed of the enzymes and observational studies have indicated that higher circulating sPLA<sub>2</sub>-IIA mass is associated with increased risk of incident and major vascular event (MVE).<sup>15</sup>

Clinical Significance

sPLA<sub>2</sub>-IIA is a cardiovascular biomarker, which aids in prediction of coronary risk and in the prognosis of patients across different cardiac risk groups. It is a strong predictor of adverse outcomes, including CVD, myocardial infarction (MI), stroke and heart failure.<sup>16</sup> Key observations through research have found that sPLA<sub>2</sub>-mediated modification of lipoproteins plays a role in the development of atherosclerosis. The surface of both LDL-C and HDL-C is surrounded by phosphatidylcholine (PC) a type of phospholipid which has been scientifically proven to serve as a good extracellular target for several isoforms of sPLA<sub>2</sub>-IIA. sPLA<sub>2</sub>-IIA works by hydrolysing these phospholipids resulting in the production of free fatty acids and lysophosphatidylcholine (LPC) which can generate pro-inflammatory actions, accelerating atherosclerosis.<sup>17</sup> Fig 8 is an illustration of the proposed role sPLA<sub>2</sub>-IIA in the development of atherosclerosis. The diagram highlights the role sPLA<sub>2</sub>-IIA has in the hydrolysis of LDL-C into the more atherogenic sdLDL-C.

Lp-PLA<sub>2</sub> vs sPLA<sub>2</sub>-IIA

Lp-PLA<sub>2</sub> is a cardiac biomarker, sharing similarities with sPLA<sub>2</sub>-IIA as it too is a member of the phospholipase A<sub>2</sub> enzyme family. Both sPLA<sub>2</sub>-IIA and Lp-PLA<sub>2</sub> have associations with LDL-C.

Though involved in similar mechanisms, research has found that among biomarkers of inflammation, sPLA<sub>2</sub>-IIA mass improved identification of patients with an increased risk of major adverse cardiovascular event.<sup>18</sup> Although Lp-PLA<sub>2</sub> mass has been associated with some cardiovascular diseases, researchers question whether Lp-PLA<sub>2</sub> has clinical utility and its role as a risk prediction biomarker.<sup>19</sup>

Findings from Key Publications:

- High levels of sPLA<sub>2</sub>-IIA can also be associated with other diseases providing more areas for testing. The risk factors associated with elevated sPLA<sub>2</sub>-IIA are diabetes, mellitus, hypertension, HDL and LDL-cholesterol.<sup>20</sup>
- Elevated concentrations of sPLA<sub>2</sub>-IIA showed a statistically significant increased risk for secondary CVD events independent of a variety of potential cofounders.<sup>21</sup>


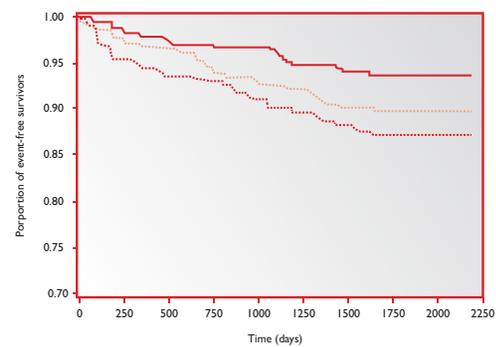


Fig. 9 Kaplan-Meier estimates of secondary fatal and non-fatal CVD events during follow-up according to tertiles of sPLA<sub>2</sub> mass at baseline. <sup>21</sup>

Key Features of the Radox sPLA<sub>2</sub>-IIA assay

- **A niche product from Radox** meaning that we are one of the only manufacturers to provide the sPLA<sub>2</sub>-IIA test in an automated chemistry form
- **Automated assay** which removes the inconvenience and time consumption associated with traditional ELISA based testing
- **Applications available** for a wide range of automated biochemistry analysers to ensure ease of programming and confidence in results
- **Liquid ready-to-use** reagents for convenience and ease-of-use
- **Latex Enhanced Immunoturbidimetric method** delivering high performance
- **Controls and calibrators available** offering a complete testing package

Fig. 8 A proposed role of sPLA<sub>2</sub>-IIA in the development of atherosclerosis <sup>16</sup>

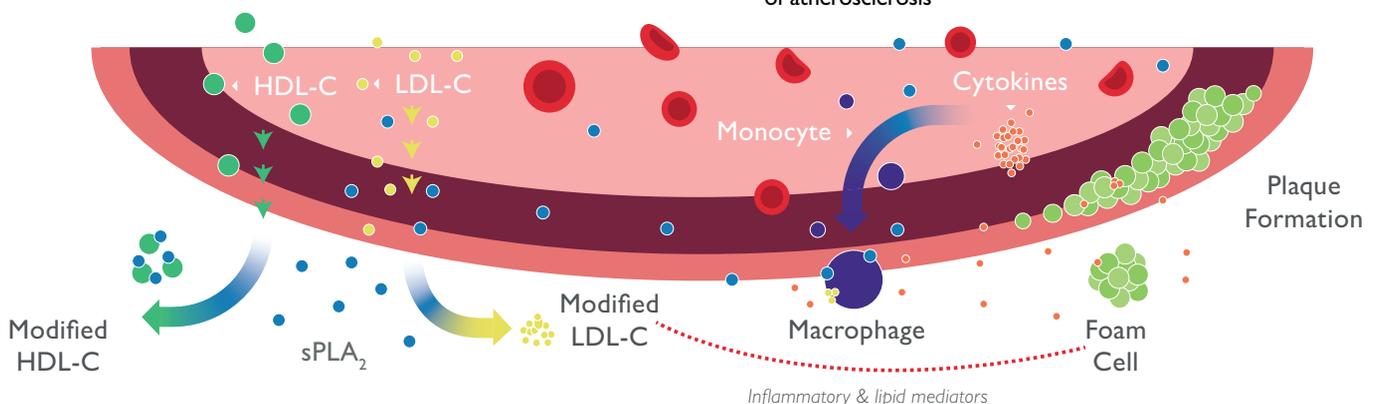



## HOMOCYSTEINE


### Key Features of the Randox Homocysteine Assay

- UF** Two shot, liquid ready-to-use reagent kit for optimum convenience
- UF** Limited interference from Bilirubin, Haemoglobin, Intralipid® and Triglycerides, producing more accurate results
  - **Calibrator is included in the kit** offering a complete testing package
  - **Wide measuring range** of 1.7 - 47.9 µmol/L. The normal range for homocysteine is approximately 5-20 µmol/L therefore the Randox assay can detect abnormal levels of homocysteine within a sample
  - **Excellent stability** of 28 days on-board the analyser when stored at +10°C, minimising reagent waste
  - **Applications available** detailing instrument-specific settings for the convenient use of the Randox Homocysteine assay on a wide range of clinical chemistry analysers

### Clinical Significance

Elevated levels of homocysteine have been shown to damage the endothelial cell wall of arteries. Damage and the associated inflammation at these sites, coupled with elevated lipoproteins can place an individual at higher risk of developing CVD through atherosclerosis. Hyperhomocysteinemia, elevated levels of homocysteine, can be associated with an increased risk of CVD. Patients with chronic renal disease experience an excess morbidity and mortality due to arteriosclerotic CVD. Elevated concentrations of homocysteine is a frequently observed finding in the blood of these patients.

**Fig. 10 2006 AHA / CDC Guidelines: hsCRP Levels vs Heart Attack Risk**

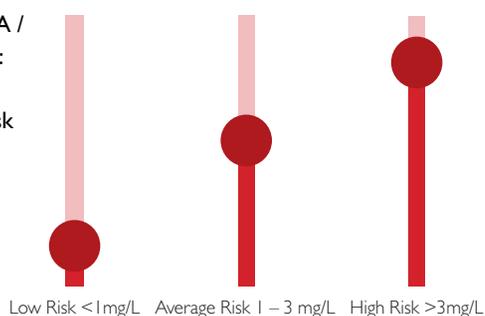

## HIGH SENSITIVITY CRP

### Key Features of the Randox High Sensitivity CRP Assay

- **Liquid ready-to-use reagents** for optimum convenience and ease-of-use
- **Latex Enhanced Immunoturbidimetric methodology** delivering high performance
- **Wide measuring range** of 0.477-10 mg/L for measurement of clinically important results
- **Limited interference** from Bilirubin, Haemoglobin, Intralipid® and Triglycerides, producing more accurate results
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox hsCRP assay on a wide range of clinical chemistry analysers

### Clinical Significance

**Risk Assessment** - High Sensitivity CRP (hsCRP) in addition to lipid evaluation and risk scoring systems aids in the assessment of cardiovascular disease (CVD) risk. Approximately half of all heart attacks occur in patients who have a normal lipid profile and are classified as **low risk based on traditional methods** of risk estimation. The measurement of hsCRP can help clinicians to identify these individuals earlier. Healthy individuals with CRP levels higher than 3mg/l are 2 to 4 times more likely to have a heart attack or stroke. It can also be used to evaluate the risk of a **recurrent cardiac event**.

**Prognosis** - In high risk groups there have been indications that CRP could be used as a prognostic tool.

**Guidelines** - The American Heart Association (AHA) and Centre for Disease Control and Prevention (CDC) recommend the use of hsCRP as a more sensitive marker of CVD risk compared to traditional CRP assays, and suggest the risk guidelines, shown in Figure 10.





## CK-MB

### Key Features of Randox CK-MB

- **Wide range of kits sizes and formats available** offering choice and minimal reagent waste
- **Liquid and lyophilised options available** to satisfy individual user requirements
- **Randox Easy Fit reagents available** which directly fit on to a wide range of analysers, including Hitachi 717, Abbott Architect and Beckman Coulter AU Series machines and are used in conjunction with validated analyser applications to ensure ease of programming
- **Randox Easy Read reagents available for Hitachi analysers** which these reagents are packaged in dedicated bottles and are barcoded for use, removing the need for any additional steps to be completed
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox CK-MB assay on a wide range of clinical chemistry analysers

## MYOGLOBIN

### Key Features of Randox Myoglobin

- **Latex Enhanced Immunospectrometric methodology** offering superior performance
- **Liquid ready-to-use reagents** for convenience and ease-of-use
- **Wide measuring range of 20.1 - 725 ng/ml** with normal levels of myoglobin being < 85 ng/ml
- **Applications available** detailing instrument specific settings for the convenient use of the Randox Myoglobin assay on a wide range of clinical chemistry analysers

## DIGOXIN

### Key Features of the Randox Digoxin Assay

- **Latex Enhanced Immunospectrometric methodology** offering superior performance
- **Liquid ready-to-use reagents** for convenience and ease-of-use
- **Excellent stability** of 21 days on-board the analyser at +2 to +8°C, minimising reagent waste
- **Applications available** detailing instrument-specific settings for the convenient use of the Randox Digoxin assay on a wide range of clinical chemistry analysers

### Clinical Significance

Digoxin is a drug commonly used to treat patients with heart failure and arrhythmias. It increases the strength of the heart's contraction. A stronger heartbeat means that the heart will circulate more blood and helps to reduce the symptoms of heart failure. Digoxin can also regulate, and slow the heart rate, and is therefore useful in certain heart rhythm disorders.

As these conditions are generally chronic, monitoring Digoxin levels is useful in managing the patient's condition.





## RANDOX MULTIPLEX BIOCHIP ARRAY TECHNOLOGY

Randox offer diagnostic and research solutions utilising our innovative Biochip Array Technology (BAT). BAT enables multi-analyte testing of biological samples to provide a complete patient profile from a single sample for rapid and accurate diagnosis.

The biochip acts as a solid phase reaction vessel, where biochips are pre-fabricated with discrete test regions (DTRs); a different antibody/oligonucleotide is immobilised at each spatially distinct DTR. Up to 49 individual DTRs can be arrayed on to a single biochip with one biochip per sample used to generate multiple results simultaneously.

The biochip detection is based on a chemiluminescent signal emitting light, without heat, as a result of a chemical reaction. The light emitted is detected and quantified using a CCD camera.

Biochip Array Technology operates via the Evidence series of analysers designed to deliver efficient high-quality testing and significant time and cost savings.

## FAMILIAL HYPER CHOLESTEROLAEMIA (FH) ARRAYS I & II

### Key Features


- Rapid turnaround time of ~3 hours from extracted genomic DNA to result
- Samples can be assessed in low batches (3 biochips) with only 20ng of genomic DNA required per array
- Ideal protocol for rapid, cost effective cascade testing in family members of FH index patient

### Patient

- Rapid mutational test to diagnose FH, the most commonly inherited lipid disease
- Mutational status can be determined rapidly from a single test, with a reduced need for confirmatory testing with NGS
- Genetic analysis for FH mutations gives a definitive diagnosis compared to lipid profiling

### Laboratory

- CE - marked IVD product.
- The array tests for 40 specific FH-causing mutations with ~78% coverage in the UK and Ireland, providing a targeted, cost-effective assay for FH testing. Rapid turnaround time allows results to be reported same day, compared to lengthy NGS screening which can take several weeks
- The array consists of 2 mutation panels, allowing for single panel testing in cases of cascade screening of known mutations for further laboratory cost savings

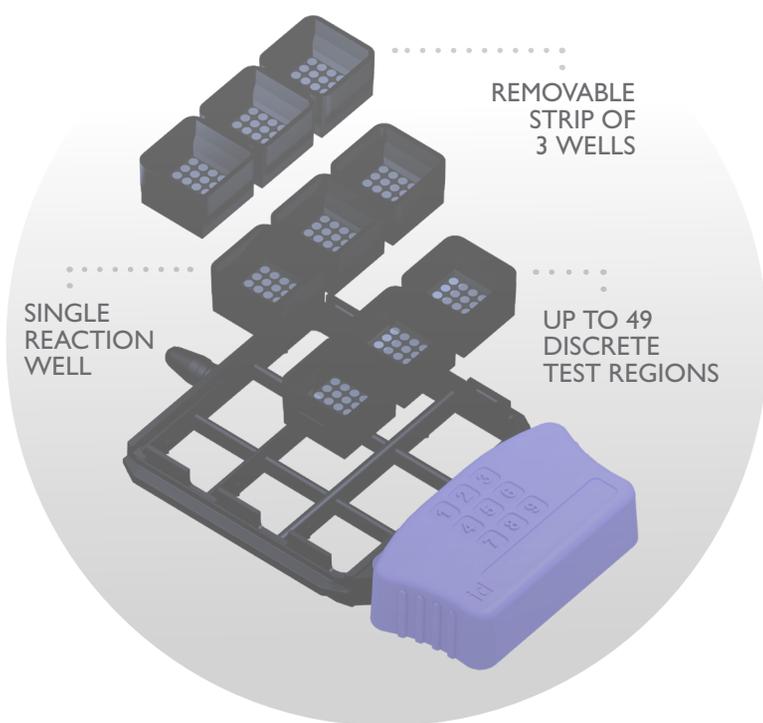



## CARDIAC RISK PREDICTION ARRAY

### Key features

- Same day genotyping of 20 GWAS - identified SNPs
- 36 patient samples can be processed per kit
- Easy to interpret results using the Randox Evidence Investigator dedicated software

### Patient

- Enhanced CHD risk assessment allows for early intervention therapeutic treatment and/or lifestyle changes to improve cardiovascular health and reduce the risk of CHD
- Genetic profiling identifies those patients predisposed to statin-induced myopathy, allowing clinicians to make more informed decisions when prescribing lipid lowering therapies

### Laboratory

- Developed with key opinion leaders in cardiovascular genetics to identify SNPs associated with CHD risk
- Uniquely combines SNP genotyping and patient questionnaire data with an algorithm to generate an easy to interpret cardiac risk score

## CARDIAC PROTEIN ARRAY

The Cardiac Array simultaneously detects up to four cardiac markers from a single patient sample, providing highly accurate quantitative results. Suitable for use within both a clinical and research setting.

ACS refers to a range of acute myocardial states, ranging from unstable angina pectoris to acute myocardial infarction (AMI) with or without ST-segment elevation. Diagnosis and risk stratification (from low risk to high risk) are closely linked in ACS.

Biochemical markers in serum are used as analytical tools for the diagnosis in conjunction with physical examination, clinical history, electrocardiogram and imaging investigations. The Randox Cardiac Array enables the simultaneous determination of four cardiac markers (including late and early markers) from a single sample thus increasing the test result output to facilitate early detection, diagnosis and therapeutic monitoring. Corresponding tri-level QC material available.

### Cardiac Array

- Creatine-Kinase Muscle Brain (CK-MB)
- Heart-Type Fatty Acid Binding Protein (H-FABP)
- Myoglobin (MYO)
- Troponin I (cTnI)

### Key benefits of Randox Cardiac Array

- Multiplex testing from a single sample
- Suitable for human serum samples
- Small sample volume

### Available on Evidence Investigator analyser

- Increased analytical information
- Improved risk stratification of patients with suspected ACS



<u>DESCRIPTION</u>	<u>METHOD</u>	<u>SIZE</u>	<u>CAT. NO.</u>
			<b>AB362</b>
Apolipoprotein A-I ♦	Immunoturbidimetric	R1 4 × 40ml, R2 4 × 17ml (S)	LP2116
Apolipoprotein A-I ♦	Immunoturbidimetric	R1 2 × 8.6ml, R2 2 × 4.8ml	LP8007
Apolipoprotein A-I ♦	Immunoturbidimetric	R1 4 × 30ml, R2 4 × 12ml	LP3838
Apolipoprotein A-II ♦	Immunoturbidimetric	R1 2 × 11ml, R2 2 × 5ml	LP3867
Apolipoprotein B ♦	Immunoturbidimetric	R1 4 × 50ml, R2 4 × 9ml (S)	LP2117
Apolipoprotein B ♦	Immunoturbidimetric	R1 2 × 8.7ml, R2 3 × 3.9ml	LP8008
Apolipoprotein B ♦	Immunoturbidimetric	R1 4 × 20ml, R2 4 × 6ml	LP3839
Apolipoprotein C-II ♦	Immunoturbidimetric	R1 2 × 11ml, R2 2 × 5ml	LP3866
Apolipoprotein C-III ♦	Immunoturbidimetric	R1 2 × 11ml, R2 2 × 5ml	LP3865
Apolipoprotein E ♦	Immunoturbidimetric	R1 2 × 11ml, R2 2 × 5ml	LP3864
CK-MB	Immunoinhibition (UV)	19 × 2.5ml	CK1296
CK-MB	Immunoinhibition (UV)	R1 4 × 20ml, R2 4 × 6ml	CK3813
CK-MB ♦	Immunoinhibition (UV)	R1 4 × 20ml, R2 4 × 6ml	CK4043
CK-MB	Immunoinhibition (UV)	R1 4 × 20ml, R2 4 × 8ml	CK8148
FH Arrays I & II	Biochip	54 biochip kit	EV3825/ EV3917A1B
Digoxin ♦	L.E.I.	R1 2 × 8ml, R2 2 × 6ml	TD3410
HDL Cholesterol ♦	Direct Clearance	R1 3 × 2.5L, R2 1 × 2.5L	CH1383
HDL Cholesterol ♦	Direct Clearance	R1 6 × 78ml, R2 3 × 52ml	CH2655
HDL Cholesterol ♦	Direct Clearance	R1 3 × 51ml, R2 3 × 20ml	CH3811
HDL Cholesterol ♦	Direct Clearance	R1 4 × 38.2ml, R2 4 × 18.2ml	CH8033
HDL Cholesterol ♦	Direct Clearance	R1 4 × 20ml, R2 4 × 9ml	CH8311
HDL Cholesterol Precipitant ♦	Phosphotungstic Acid	4 × 80ml	CH203*
High Sensitivity CRP ♦	L.E.I.	R1 2 × 11ml, R2 2 × 11ml	CP3885
Homocysteine ♦	Enzymatic	R1 2 × 21.7ml, R2 2 × 4.6ml (S)	HY4036
LDL Cholesterol ♦	Direct Clearance	R1 6 × 78ml, R2 3 × 52ml	CH2656
LDL Cholesterol ♦	Direct Clearance	R1 6 × 30ml, R2 3 × 20ml	CH2657
LDL Cholesterol ♦	Direct Clearance	R1 3 × 51ml, R2 3 × 20ml	CH3841
LDL Cholesterol ♦	Direct Clearance	R1 4 × 19.2ml, R2 4 × 10.1ml	CH8032
LDL Cholesterol ♦	Direct Clearance	R1 4 × 20ml, R2 4 × 9ml	CH8312
Lipoprotein(a) ♦	L.E.I.	R1 1 × 30 ml, R2 1 × 15 ml	LP2757
Lipoprotein(a) ♦	L.E.I.	R1 1 × 10 ml, R2 1 × 6 ml	LP3403
Lipoprotein(a) ♦	L.E.I.	R1 2 × 8.7ml, R2 2 × 5.8ml	LP8054
Myoglobin ♦	L.E.I.	R1 1 × 9.5ml, R2 1 × 4.5ml	MY2127
sdLDL Cholesterol ♦	Direct Clearance	R1 1 × 16.2 ml, R2 1 × 8.2 ml	CH8153

<u>DESCRIPTION</u>	<u>METHOD</u>	<u>SIZE</u>	<u>CAT. NO.</u>
			
sdLDL Cholesterol ♦	Direct Clearance	R1 1 × 19.8ml R2 1 × 8.6ml	562616
sdLDL Cholesterol (U) ♦	Direct Clearance	R1 1 × 18ml R2 1 × 7ml	562760
sdLDL Cholesterol (U) ♦	Direct Clearance	R1 5 × 200ml R2 2 × 200ml	562791, 562807
Total Cholesterol ♦	CHOD-PAP	6 × 30ml (S)	CH200
Total Cholesterol ♦	CHOD-PAP	6 × 100ml (S)	CH201
Total Cholesterol ♦	CHOD-PAP	9 × 51ml	CH3810
Total Cholesterol ♦	CHOD-PAP	4 × 68ml	CH8019
Total Cholesterol ♦	CHOD-PAP	4 × 20ml	CH8310
Triglycerides	GPO-PAP	6 × 15ml (S)	TR210
Triglycerides	GPO-PAP	4 × 100T (S)	TR1697
Triglycerides	GPO-PAP	6 × 51ml	TR3823
Triglycerides	GPO-PAP	4 × 58ml	TR8067
Triglycerides ♦	GPO-PAP	8 × 20ml	TR8147
Triglycerides ♦	GPO-PAP	4 × 20ml	TR8332
Triglycerides	GPO-PAP	4 × 60ml	TR9780

\* Precipitant for use with CH200, CH201 and CH202

♦ Indicates liquid option available

(S) Indicates standard included in kit

(U) USA Only

1. CVD Risk Stratification in the PCSK0 Era: Is There a Role for LDL Subfractions? Kjellmo, Christian, Hovland, Anders and Lappegard, Knut. 2, s.l. : MDPI, 2018, Vol. 6.
2. Izawa, S., Okada, M., Matsui, H. and Horita, Y. A new direct method for measuring HDL cholesterol which does not produce any biased values. *Journal of Medical and Pharmaceutical Science*. Vol. 37, p. 1385–1388 (1997) (Adapted)
3. Cohen et al (1997) *Canadian Journal of Cardiology* 13B No. 0762\*\*
4. Hirano, T. Ito, Y. and Yoshino, G. Measurement of small dense low density lipoprotein particles. *J Atherosclerosis Thromb*. Vol. 12, no. 2, p. 67-72 (2005).
5. Austin, M.A., Breslow, J. L., Hennekens, C.H., Buring, J.E., Willett, W. C. and Krauss, R.M. LDL subclass patterns and risk of MI. *JAMA*. Vol. 260, no. 13, p. 1917-21 (1988).
6. Teng Leary, E., Ph.D. AACC Presentation by Pacific Biometrics. AACC Annual Scientific Meeting & Clinical Lab Expo; 2006 Jul 23-27; Chicago, IL (Adapted).
7. Mora. S. (2006). LDL Particle Size: Does It Matter?'. Harvard Medical School. Boston, MA.
8. Marcovina, S.M. and Albers, J.J. Lipoprotein (a) measurements for clinical application. *Lipid Res*. Vol. 57, p. 526-37 (2016).
9. Kamstrup P.R., Tybjaerg-Hansen A., Steffensen R., Nordestgaard B.G. Genetically elevated lipoprotein (a) and increased risk of myocardial infarction. *JAMA*. Vol. 301, p. 2331-2339 (2009).
10. Joshi, P. H., Toth, P. P., Lirette, S. T., Griswold, M. E., Massaro, J. M., Martin, S. S., Blaha, M. J., Kulkarni, K. R., Khokhar, A. A., Correa, A., D'Agustino Sr, R. B., and Jones, S. R. on behalf of the Lipoprotein Investigators Collaborative (LIC) Study Group. Association of high-density lipoprotein subclasses and incident coronary heart disease: The Jackson Heart and Framingham Offspring Cohort Studies. *Eur J Prev Cardiol*. Vol. 23, no. 1, p. 41 – 49 (2016).
11. Tremulis. S. 2018, Lipoprotein(a) Foundation Announces Two ICD-10 Diagnostic Codes for Elevated Lipoprotein(a) approved by the CDC. Available at: <https://www.lipoproteinafoundation.org/news/407398/CDC-grants-ICD-10-Codes-of-Elevated-Lipoproteina.htm> (Accessed: 27th November 2018)
12. Albers, J. J., Slee, A., Fleg, J. L., O'Brien, K. D., Marcovina S. M. Relationship of baseline HDL subclasses, small dense LDL and LDL triglyceride to cardiovascular events in the AIM-HIGH clinical trial. *Atherosclerosis*. Vol. 251, p. 454 – 459, (2016).
13. Martin, S. S., Khokhar, A. A., May, H. T., Kulkarni, K. R., Blaha, M. J., Joshi, P. H., Toth, P. P., Muhlestein, J. B., Anderson, J. L., Knight, S., Li, Y., Spertus, J. A., and Jones, S. R., on behalf of the Lipoprotein Investigators Collaborative (LIC). HDL cholesterol subclasses, myocardial infarction, and mortality in secondary prevention: the lipoprotein investigators collaborative. *European Heart Journal*. Vol. 36, p. 22–30 (2015).
14. Joshi, P. H., Toth, P. P., Lirette, S. T., Griswold, M. E., Massaro, J. M., Martin, S. S., Blaha, M. J., Kulkarni, K. R., Khokhar, A. A., Correa, A., D'Agustino Sr, R. B., and Jones, S. R. on behalf of the Lipoprotein Investigators Collaborative (LIC) Study Group. Association of high-density lipoprotein subclasses and incident coronary heart disease: The Jackson Heart and Framingham Offspring Cohort Studies. *Eur J Prev Cardiol*. Vol. 23, no. 1, p. 41 – 49 (2016).
15. Role of secretory phospholipase A2 in women with metabolic syndrome. Pop, D. et al. 6, s.l. : Indian Journal of Medical Research, 2013, Vol. 138.
16. Secretory Phospholipase A2-IIa and Cardiovascular Disease. Holmes, Michael, Simon, Tabassome and Exeter, Holly. 21, 2013, Vol. 62.
17. Secreted phospholipase A2, lipoprotein hydrolysis, and atherosclerosis: integration with lipidomics. Kei, Yamamoto, et al. 7, s.l. : Analytical and Bioanalytical Chemistry, 2011, Vol. 400.
18. Prognostic Utility of Secretory Phospholipase A2 in Patients with Stable Coronary Artery Disease. O'Donoghue , Michelle, Mallat, Ziad and Morrow, David. 9, s.l. : Clinical Chemistry, 2011, Vol. 57.
19. Clinical utility of lipoprotein associated phospholipase A2 for cardiovascular disease prediction in multi-ethnic cohort of women. Cook, Nancy, Paynter, Nina and Manson, JoAnn. 9, s.l. : NCBI, 2012, Vol. 58.
20. Serum Secretory phospholipase A2-IIa levels in patients surviving acute myocardial. Xin, H, et al. 8], s.l. : NCBI, 2013, Vol. 17.
21. Association between type II secretory phospholipase A2 plasma concentrations and activity and cardiovascular events in patients with coronary heart disease. Wolfgang, Koenig. et al. 22, s.l. : European Heart Journal, 2009, Vol. 30
22. Tsimikas, S., Mallat, Z., MD, Talmud, P. J., Kastelein, J. J. P., Wareham, N. J., Sandhu, M. S., Miller, E. R., Benessiano, J., Tedgui, A., Witztum, J. L., Khaw, K. T. and Boekholdt, S. M. (2010). Oxidation-Specific Biomarkers, Lipoprotein(a), and Risk of Fatal and Nonfatal Coronary Events. *JACC*. 56:12, p. 946-955.
23. Ai, M., Otokozaawaw, S., Asztalos, B. F., White, C., Cupples, L. A., Nakajima, K., Lamon-Fava,
24. Persson, J., Lindberg, K., Gustafsson, T. P., Eriksson, P., Paulsson-Berne, G. and Lundman, P. Low plasma adiponectin concentration is associated with myocardial infarction in young individuals. *Journal of Internal Medicine*. Vol. 268, no. 2, p. 194-205 (2010).
25. Jung, D. H., Kim, J. Y., Kim, J. K., Koh, S. B., Park, J. K. and Ahn, S. V. Relative contribution of obesity and serum adiponectin to the development of hypertension. *Diabetes Res. Clin. Practise*. Vol. 103, no. 1, p. 51-6 (2014).
26. Brambilla, P., Antolini, L., Street, M. E., Giussani, M., Galbiati, S., Valsecchi, M. G., Stella, A., Zucotti, G. V., Bernasconi, S. and Genovesi, S. Adiponectin and hypertension in normal-weight and obese children. *Am. J. Hypertens*. Vol. 26, no. 2, p. 257-64 (2013).
27. McMahan, C.G., Lamont, J.V., Curtin, E., McConnell, R.I., Crockard, M., Kurth, M.J., Crean, P. and Fitzgerald, S.P. Diagnostic accuracy of heart-type fatty acid-binding protein for the early diagnosis of acute myocardial infarction. *Am J Emerg Med*. Vol. 30, no. 2, p. 267-74 (2012).
28. Menzaghi, C., Trischitta, V. and Doria, A. Genetic Influences of Adiponectin on Insulin Resistance, Type 2 Diabetes, and Cardiovascular Disease. *Perspectives in Diabetes*, vol. 56, p. 1198-1209 (2007).
29. Glatz, J.F.C., van Bilsen, M., Paulussen, R.J.A., Veerkamp, J., van der Vusse, G.J. and Reneman, R.S. Release of fatty acid-binding protein from isolated rat heart subjected to ischemia and reperfusion or the calcium paradox. *Biochim Biophys Acta*. Vol. 961, p. 148-52 (1988).
30. McCann, C.J., Glover, B.M., Menown, I.B., Moore, M.J., McEnery, J., Owens, C.G., Smith, B., Sharpe, P.C., Young, I.S. and Adgey, J.A. Prognostic value of a multimarker approach for patients presenting to hospital with acute chest pain. *Am J Cardiol*. Vol. 103, no. 1, p. 22-8 (2009).
31. Body, R., McDowell, G., Carley, S., Wibberley, C., Ferguson, J. and Mackway-Jones, K. A FABP-ulous 'rule out' strategy? Heart fatty acid binding protein and troponin for rapid exclusion of acute myocardial infarction. *Resuscitation*. Vol. 82, no. 8, p. 1041-6 (2011).
32. McCann, C.J., Glover, B.M., Menown, I.B., Moore, M.J., McEnery, J., Owens, C.G., Smith, B., Sharpe, P.C., Young, I.S. and Adgey, J.A. Novel biomarkers in early diagnosis of acute myocardial infarction compared with cardiac troponin T. *Eur Heart J*. Vol. 29, no. 23, p. 2843-50 (2008).
33. Reddy, L.L., Shah, S.A., Dherai, A.J., Ponde, C.K. and Ashavaid, T.F. Troponin T and heart type fatty acid binding protein (h-Fabp) as biomarkers in patients presenting with chest pain. *Indian J Clin Biochem*. Vol. 31, no. 1, p. 87-92 (2016).

34. Ghani, F., Wu, A., Graff, L., Petry, C., Armstrong, G., Prigent, F. and Brown, M. Role of heart-type fatty acid-binding protein in early detection of acute myocardial infarction. *Clin Chem.* Vol. 46, p. 718-719 (2000).
  35. Pelsers, M.M., Hermens, W.T. and Glatz, J.F. Fatty acid-binding proteins as plasma markers of tissue injury. *Clin. Chem. Acta.* Vol. 352, no. 1-2, p. 15-35 (2005).
  36. kleine, A.H., Glatz, J.F., van Nieuwenhoven, F.A. and van der Vasse, G.J. Release of heart type fatty acid binding protein into plasma after acute myocardial infarction in man. *Mol Cell Biochem.* Vol. 116, p. 155-162 (1992).
-

## A-Z PORTFOLIO OF REAGENTS

Albumin	Digoxin	Rheumatoid Factor (RF)
Aldolase	Ethanol	Sodium
Alkaline Phosphatase	Ferritin	sPLA <sub>2</sub> -IIA
Alanine Aminotransferase (ALT)	Fructosamine	Soluble Transferrin Receptor (sTfR)
Ammonia	G6PDH	Superoxide Dismutase (Ransod)
Amylase (Pancreatic)	Gamma GT	Syphilis
Anti-Streptolysin O (ASO)	GLDH	Total Iron Binding Capacity (TIBC)
Apolipoprotein A-I	Glucose	Total Antioxidant Status (TAS)
Apolipoprotein A-II	Glutamate	Total Protein
Apolipoprotein B	Glutamine	Transferrin
Apolipoprotein C-II	Glutathione Peroxidase (Ransel)	Transthyretin (Prealbumin)
Apolipoprotein C-III	Glutathione Reductase	Triglycerides
Apolipoprotein E	Glycerol	Urea
Aspartate Aminotransferase (AST)	Haemoglobin	Uric Acid
β2 Microglobulin	Haptoglobin	Urinary Protein
Bile Acids	HbA1c	Valproic Acid
Bilirubin (Direct)	HbA1c II	Zinc
Bilirubin (Total)	Homocysteine	
Calcium	D-3-Hydroxybutyrate (Ranbut)	
Carbamazepine	IgA	
Cholesterol (Total)	IgE	
Cholesterol (HDL)	IgG	
Cholesterol (LDL)	IgM	
Cholesterol (sdLDL)	Iron	
Cholinesterase	L-Lactate	
CK-MB	Lactate Dehydrogenase L-P	
CK-NAC	Lactate Dehydrogenase P-L	
CO <sub>2</sub> Total	Lipase	
Complement C3	Lipoprotein (a)	
Complement C4	Magnesium	
Copper	Microalbumin	
Creatinine	Myoglobin	
CRP	NEFA (Non-Esterified Fatty Acids)	
CRP (Canine)	Phenobarbital	
CRP (Full Range)	Phenytoin	
CRP (High Sensitivity)	Phosphorus	
Cystatin C	Potassium	

## RANDOX - A GLOBAL DIAGNOSTIC SOLUTIONS PROVIDER

Randox has been supplying laboratories worldwide with revolutionary diagnostic solutions for over 40 years. Our experience and expertise allow us to create a leading product portfolio of high quality diagnostic tools which offer reliable and rapid diagnosis. We believe that by providing laboratories with the right tools, we can improve health care worldwide.



### RX SERIES

Renowned for quality and reliability, the RX series combines robust hardware and intuitive software with the world leading RX series test menu comprising an extensive range of high quality reagents including routine chemistries, specific proteins, lipids, therapeutic drugs, drugs of abuse, antioxidants and diabetes testing. The RX series offers excellence in patient care delivering unrivalled precision and accuracy for results you can trust, guaranteeing real cost savings through consolidation of routine and specialised tests onto one single platform.



### INTERNAL QUALITY CONTROL

Acusera third party quality controls are made using the highest quality material of human origin, ensuring they react like a real patient sample. With more than 390 analytes available across the Acusera range we can uniquely reduce the number of controls required while reducing costs and time. Our product range includes clinical chemistry, immunoassay, urine, immunology and more. Qnostics molecular controls for infectious disease testing are designed to meet the demand of today's molecular diagnostics laboratory while effectively monitoring the entire testing process. Our whole pathogen molecular controls comprise hundreds of characterised viral, bacterial and fungal targets.



### EXTERNAL QUALITY ASSESSMENT

RIQAS is the world's largest international EQA scheme with more than 45,000 participants worldwide. 33 comprehensive, yet flexible programmes cover a wide range of clinical diagnostic testing including chemistry, immunoassay, cardiac, urine, serology and more. Our programmes benefit from a wide range of concentrations, frequent reporting, rapid feedback and user-friendly reports. The QCMD range of molecular infectious disease EQA programmes feature a whole pathogen matrix ensuring a true test of patient sample analysis. With access to over 90 programmes including blood borne viruses, respiratory diseases, multi-pathogen infections and more, there is something for every laboratory.



### EVIDENCE SERIES

In 2002, Randox invented the world's first, Biochip Array Technology, offering highly specific tests, coupled to the highly sensitive chemiluminescent detection, providing quantitative results instantly changing the landscape of diagnostic testing forever. The Randox Evidence Series of multi-analyte immunoanalyser's provide an unrivalled increase in patient information per sample offering diagnostic, prognostic and predictive solutions across a variety of disease areas with a highly advanced clinical and toxicology immunoassay test menu including cardiac, diabetes, drugs of abuse, metabolic and renal markers.

## CONTACT US

Contact us for more information on any of our products and services:

## HEADQUARTERS

Randox Laboratories Ltd, 55 Diamond Road, Crumlin, County Antrim, BT29 4QY, United Kingdom

☎ +44 (0) 28 9442 2413    ✉ reagents@randox.com    🌐 randox.com

## INTERNATIONAL OFFICES



**AUSTRALIA**  
Randox (Australia) Pty Ltd.  
Tel: +61 (0) 2 9615 4640



**BRAZIL**  
Randox Brasil Ltda.  
Tel: +55 11 5181-2024



**CHINA**  
Randox Laboratories Ltd.  
Tel: +86 021 6288 6240



**CZECH REPUBLIC**  
Randox Laboratories S.R.O.  
Tel: +420 2 1115 1661



**FRANCE**  
Laboratoires Randox  
Tel: +33 (0) 130 18 96 80



**GERMANY**  
Randox Laboratories GmbH  
Tel: +49 (0) 215 1937 0611



**HONG KONG**  
Randox Laboratories Hong Kong Limited  
Tel: +852 3595 0515



**ITALY**  
Randox Laboratories Ltd.  
Tel: +39 06 9896 8954



**INDIA**  
Randox Laboratories India Pvt Ltd.  
Tel: +91 80 6751 5000



**POLAND**  
Randox Laboratories Polska Sp. z o.o.  
Tel: +48 22 862 1080



**PORTUGAL**  
Irandox Laboratorios Quimica Analitica Ltda  
Tel: +351 22 589 8320



**PUERTO RICO**  
Clinical Diagnostics of Puerto Rico, LLC  
Tel: +1 787 701 7000



**REPUBLIC OF IRELAND**  
Randox Teoranta  
Tel: +353 7495 22600



**SLOVAKIA**  
Randox S.R.O.  
Tel: +421 2 6381 3324



**SOUTH AFRICA**  
Randox Laboratories SA (Pty) Ltd.  
Tel: +27 (0) 11 312 3590



**SOUTH KOREA**  
Randox Korea  
Tel: +82 (0) 31 478 3121



**SPAIN**  
Laboratorios Randox S.L.  
Tel: +34 93 475 09 64



**SWITZERLAND**  
Randox Laboratories Ltd. (Switzerland)  
Tel: +41 41 810 48 89



**UAE**  
Randox Medical Equipments Trading LLC  
Tel: +971 55 474 9075



**USA**  
Randox Laboratories - US, Ltd.  
Tel: +1 304 728 2890



**VIETNAM**  
Randox Laboratories Ltd. Vietnam  
Tel: +84 (0) 8 3911 0904

**FOR TECHNICAL SUPPORT CONTACT:**

technical.services@randox.com

**RANDOX**  
REAGENTS



LT147 OCT21